



POLICE DEPARTMENT

FIELD UNIT INSPECTION REPORT
INTOXILYZER 5000EN

Technical Supervisor P. Zippo (PA)

Location 45 Pct.

Date of Inspection 7/29/08

Intoxilyzer Serial # 68-011196 Simulator Serial # DE2679 Lot # 08070

- 1. .098
- 2. .098
- 3. .097
- Diagnostic test OK
- Breath hose heated OK
- Printer check OK

Intoxilyzer Serial # 68-010779 Simulator Serial # DE3561 Lot # 08070

- 1. _____
- 2. _____
- 3. _____
- Diagnostic test _____
- Breath hose heated See below
- Printer check _____




REMARKS:

Placed @ 0/0/s due to Int. Detected/in possible fan Internal temp @ 50.8°C. Hyg District notified.

(Signature)

Obtained by Perlmutter & McGuinness, P.C. in Law Offices of Adam D. Perlmutter, P.C. v. NYPD, et al., Case No. 100220/2012 (N.Y. City S. Ct.). WWW.NEWYORKLEGALDEFENSE.COM - (212) 679-1990

Obtained by Perlmutter & McGuinness, P.C. in Law Offices of Adam D. Perlmutter, P.C. v. NYPD, et al.,
Case No. 100220/2012 (N.Y. Cty. S. Ct.) WWW.NEWYORKLEGALDEFENSE.COM - (212) 679-1990

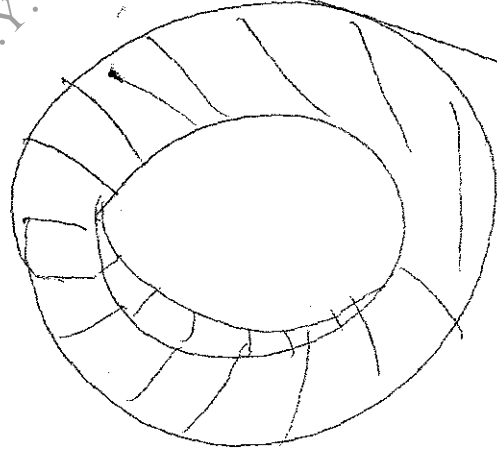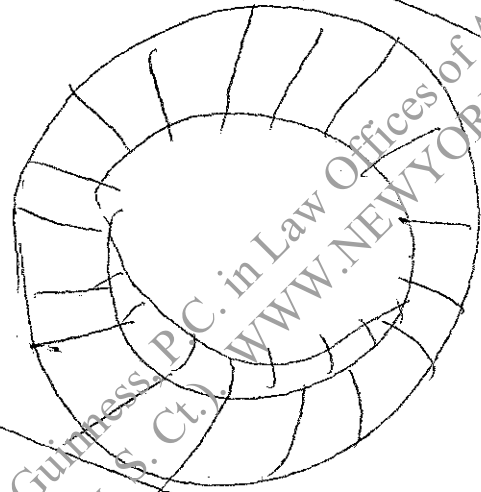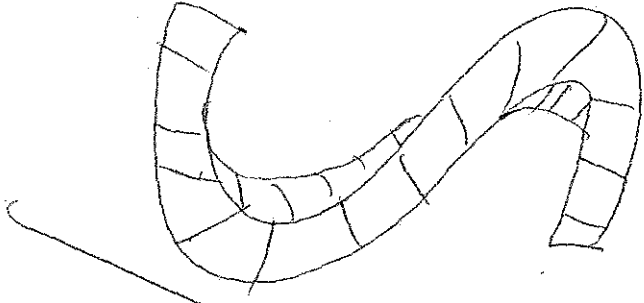

IOTC

045 PCT
INTOXILYZER - ALCOHOL ANALYZER
MODEL 5000EN SN 68-010779
07/29/2008

DIAGNOSTIC TEST 15:52 EDT

PROM CHECK	PASSED
Z80 VER - G1776.12	
SLAVE 75_2240	
RAM CHECK	PASSED
TEMP CHECK	PASSED
PROCESSOR CHECK	
MOTOR CHECK	PASSED
EEPROM CHECK	PASSED
SERIAL NO. MATCH	PASSED
RANGE/STABILITY	PASSED
AUTO CAL STATUS	PASSED

RTC CHECK	PASSED
INTERNAL STD	PASSED

DIAGNOSTIC	PASSED
------------	--------

PRINTER CHECK
ABCDEFGHIJKLMNORSTUVWXYZ
0123456789

Obtained by Perlmutter & McGuinness, P.C. in Law Offices of Adam D. Perlmutter, P.C. v. NYPD, et al.,
Case No. 100220/2012 (N.Y. Cty. S. Ct.). WWW.NEYORKLEGALDEFENSE.COM - (212) 679-1990

SN 68-010779
SLAVE 75 2240
DATE 07/29/2008
INVALID TEST
INTERFERENT DETECTED

VERSION G1776.12

TIME 15:54 EDT

Int. Temp. 50.8°C
Fan in pencil

Obtained by Perlmutter & McGuinness, P.C. in Law Offices of Adam D. Perlmutter, P.C. v. NYPD, et al.
Case No. 100220/2012 (N.Y. Cty. S. Ct.). WWW.NEWYORKLEGALDEFENSE.COM - (212) 679-1996